INSTALLATION INSTRUCTION FOR INSTRUMENT TRAY P/N (9A95001) USED ON PODIATRY TABLES #414, 416 & 417

1. POSITION CHAIR WITH BASE FULLY EXTENDED & TILT INCLINED 30°.
2. DISCONNECT THE TABLES ELECTRICAL SUPPLY CORD TO PREVENT ELECTRICAL SHOCK. FAILURE TO DO SO COULD RESULT IN PERSONAL INJURY OR EQUIPMENT DAMAGE.
3. LOOKING AT THE FRONT OF THE CHAIR, LOCATE THE TWO MOUNTING HOLES IN THE UPPER PORTION OF THE PLASTIC BASE SHROUDING. (JUST BELOW CHAIR TOP.)
4. FASTEN MOUNT WELDMENT SECURELY USING THE TWO 3/8"' BOLTS SUPPLIED.
6. POSITION TRAY ASSEMBLY AS IN FIG. BELOW. (NOTE: TRAY CAN BE ROTATED 360 DEGREES.)

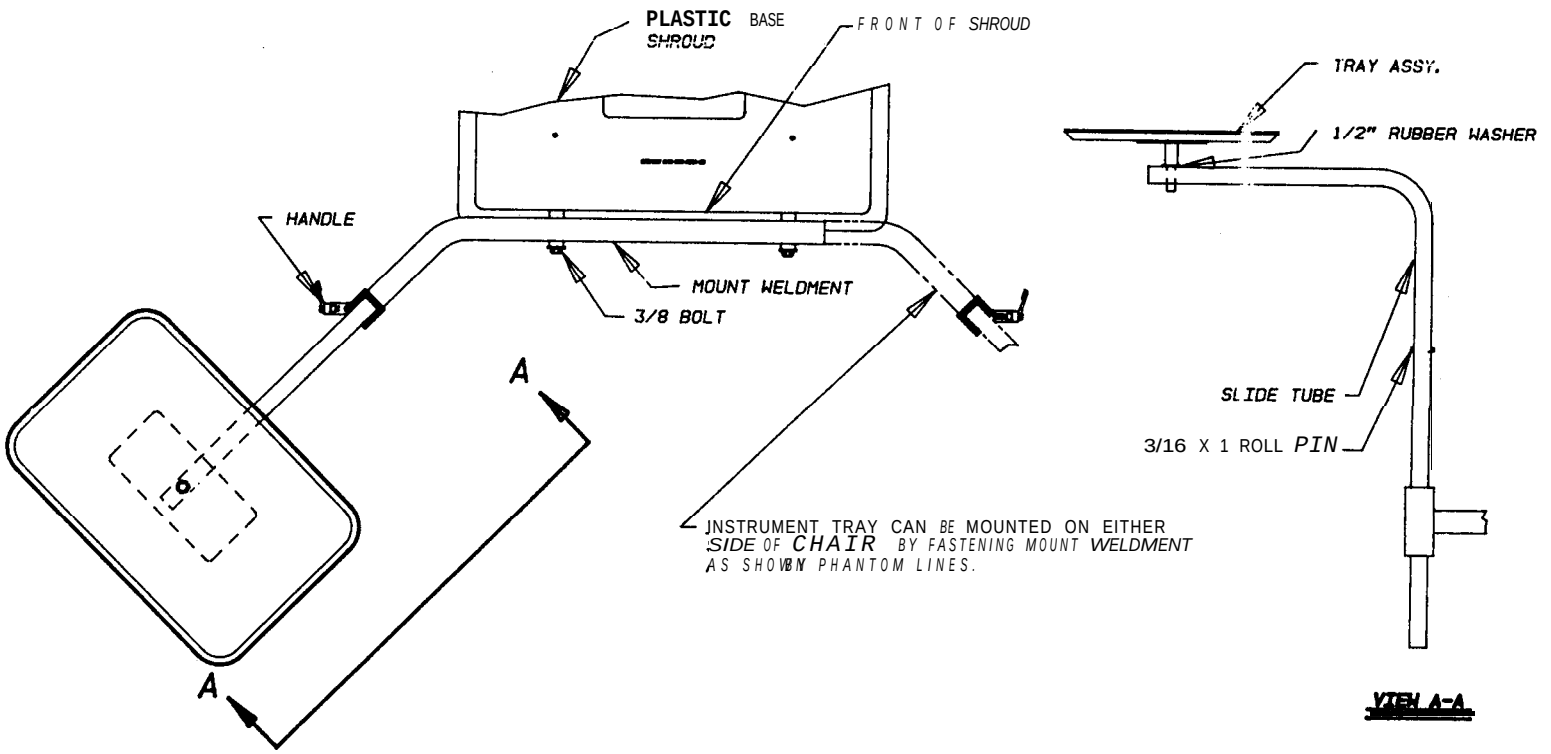

MIDMARK CORPORATIONS
VESAILLES. OHIO 45380 937-526-3362

ALL PRODUCT SUBJECT TO IMPROVEMENT CHANGES WITHOUT NOTICE!

003-0489-00 Rev. B (8/98)